

## Review

## Recent progress in the fabrication techniques of 3D scaffolds for tissue engineering

Mostafa Mabrouk<sup>a,b,\*</sup>, Hanan H. Beherei<sup>a</sup>, Diganta B. Das<sup>b</sup><sup>a</sup> Refractories, Ceramics and Building Materials Department, National Research Centre, 33El Bohouth St (Former EL Tahrirst)-Dokki, P.O. 12622, Giza, Egypt<sup>b</sup> Department of Chemical Engineering, Loughborough University, Loughborough LE113TU, Leicestershire, UK

## ARTICLE INFO

## Keywords:

Tissue engineering  
Scaffold preparation techniques  
Electrospinning  
3D printing

## ABSTRACT

Significant advances have been made in the field of tissue engineering (TE), especially in the synthesis of three-dimensional (3D) scaffolds for replacing damaged tissues and organs in laboratory conditions. However, the gaps in knowledge in exploiting these techniques in preclinical trials and beyond and, in particular, in practical scenarios (e.g., replacing real body organs) have not been discussed well in the existing literature. Furthermore, it is observed in the literature that while new techniques for the synthesis of 3D TE scaffold have been developed, some of the earlier techniques are still being used. This implies that the advantages offered by a more recent and advanced technique as compared to the earlier ones are not obvious, and these should be discussed in detail. For example, one needs to be aware of the reason, if any, behind the superiority of traditional electrospinning technique over recent advances in 3D printing technique for the production of 3D scaffolds given the popularity of the former over the latter, indicated by the number of publications in the respective areas. Keeping these points in mind, this review aims to demonstrate the ongoing trend in TE based on the scaffold fabrication techniques, focusing mostly, on the two most widely used techniques, namely, electrospinning and 3D printing, with a special emphasis on preclinical trials and beyond. In this context, the advantages, disadvantages, flexibilities and limitations of the relevant techniques (electrospinning and 3D printer) are discussed. The paper also critically analyzes the applicability, restrictions, and future demands of these techniques in TE including their applications in generating whole body organs. It is concluded that combining these knowledge gaps with the existing body of knowledge on the preparation of laboratory scale 3D scaffolds, would deliver a much better understanding in the future for scientists who are interested in these techniques.

## 1. Introduction

Tissue engineering (TE) approaches have demonstrated impressive results for the treatment and substitution of damaged tissues and organs including skin, heart, and kidney tissues, in addition to their potential to address some inherent bone defects [1–10]. When different scientific fields, e.g., materials science, biology and engineering are combined together in an interdisciplinary manner with a view to augment or regenerate malfunctioned human parts, it promises to improve the success of the TE approaches [11–16]. For the TE systems to be fruitful, the material utilized should generally be a mixture of scaffolds, growth factors, and cells. They should also most certainly be able to replace the damaged tissue and have the capacity to either work as the native tissue or mimic the native tissue [17–22].

Application of growth factors and exogenous materials with the sole

aim of quickening and enhancing the body's healing procedures could improve the tissue condition. Materials that simulate the properties of extracellular matrix have been used for a long period time till now, which accomplish more advantages other than supplying the physical structure [23–25]. Biomimetic materials can induce recovery of all, and they can be utilized for transport of biomolecules, for example, growth factors that facilitate cells growth [18,20,24–26]. At first, it was thought that scaffolds are fundamental for cells' physical support, the biomaterial or scaffold can now be loaded with biological factors to facilitate tissue recovery [27–29]. Because of the diverse recovery limits of various tissues, some tissues do not demand cells but rather simply the biomaterial and biological molecules. On the other hand, other tissues have restricted recovery limits and demand the biomaterial, biomolecules, and cells for recovery to happen. There are tissues and organs with constrained or no possibility for recovery like ligament and

\* Corresponding author at: Refractories, Ceramics and Building Materials Department, National Research Centre, 33El Bohouth St (Former EL Tahrirst)-Dokki, P.O. 12622, Giza, Egypt.

E-mail address: [mostafamabrouk.nrc@gmail.com](mailto:mostafamabrouk.nrc@gmail.com) (M. Mabrouk).

<https://doi.org/10.1016/j.msec.2020.110716>

Received 23 November 2019; Received in revised form 29 January 2020; Accepted 1 February 2020

Available online 03 February 2020

0928-4931/ © 2020 Published by Elsevier B.V.

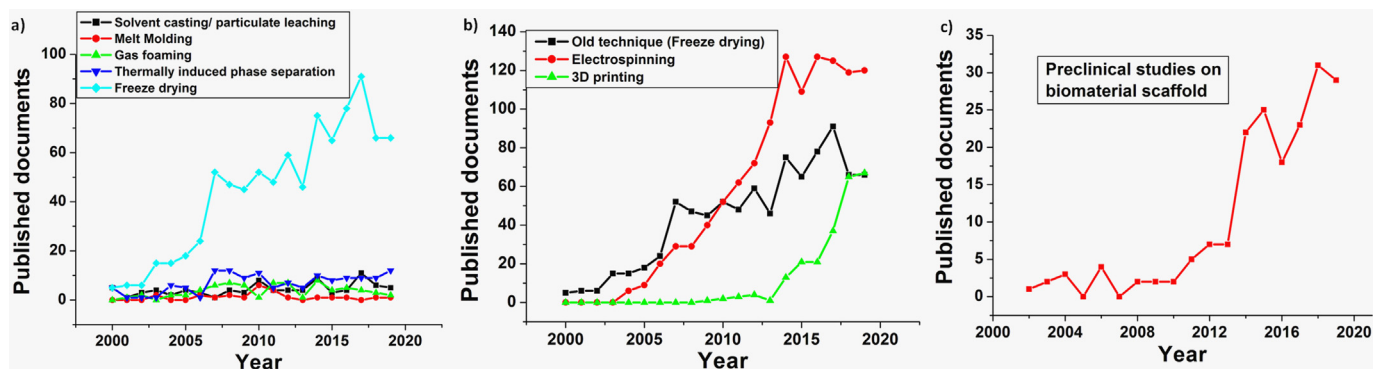


Fig. 1. Demonstrates the data obtained from *Scopus* on scaffolds preparation method for a) traditional techniques, b) advanced techniques and c) preclinical studies using biomaterial scaffold.

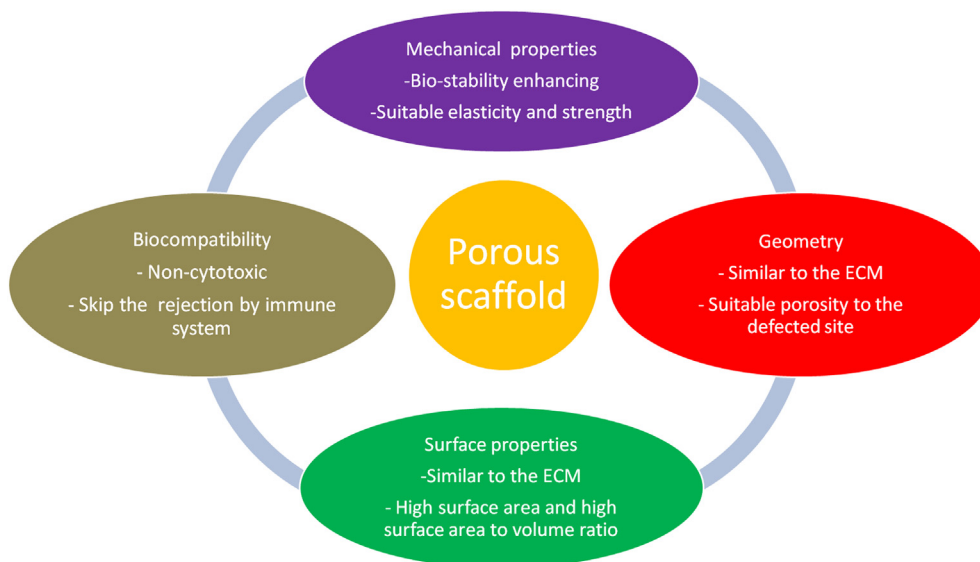


Fig. 2. Schemes representing ideal porous scaffold properties.

cornea while others have great recovery capabilities such as the liver and the lungs tissues [30,31].

Based on most of the stated research articles dealing with TE, it is obvious that the scaffold preparation techniques are important factors in this field. According to the data that have been obtained from the *Scopus* (Fig. 1), it can be seen that up till now there are a number of traditional scaffold fabrications techniques (e.g., freeze drying) which are still being utilized (see, Fig. 1a). Also, it is obvious that there are an increasing number of publications recorded for scaffolds that have been synthesized using electrospinning technique when compared with those that have been synthesized using 3D printing technique (Fig. 1b), even though both techniques have originated at similar starting time.

It is also obvious that although there are different review articles that have discussed scaffolds in TE, they have different focuses such as the nature of scaffold material and its effect on the cell growth or healing of the damaged site [11]. Other review papers consider issues on combining both inorganic and organic materials together and what are their effects on the healing rate of hard tissue [15]. Reports have also been published that suggest that these studies have handled the materials design and its effect on the regeneration of soft tissues [21], while other reports the successful clinical trials for TE from a medicinal prospect [22]. However, there is a lack of review papers that specifically highlights the effects of the scaffold fabrication techniques and how they have progressed from the early beginning up till now with the progress on TE as an engineering process, their limitations, challenges and future aspects. Therefore, the main objective of the current review

is to focus on the implemented techniques in TE field for synthesis of scaffolds, stressing out the unclear points in this specialty. In particular, this review focuses on discussing the two most widely used techniques, namely, electrospinning and 3D printing. Finally, the paper discusses briefly the applicability, restrictions, and future demands of these advanced techniques in the TE field including their applications in generating whole body organs.

## 2. Scaffold properties

Scaffolds support cells with the reasonable surviving conditions, ideal oxygen and nutrient levels, successful supplement and waste transport in addition to providing adequate mechanical support. The necessary environmental 3D conditions for cells in order to arrange or to shape tissues are also attained using 3D scaffolds. The cells must produce their own extracellular matrix (ECM) at the same time that is consumed for the scaffold biodegradation to deliver identical 3D microstructures for the damaged sites. In fact, numerous parameters influence the choice and properties of the scaffolds. Generally, the scaffolds should be biocompatible, have suitable porosity, properties of surface and neutral pH, surface charge, biodegradable, good physico-mechanical characteristics, and preferred for cells adhesion. A few necessities have been distinguished as essential for the synthesis of scaffolds [32] as summarized in Fig. 2. It is worth highlighting that the scaffold properties could be manipulated through selection of the proper preparation technique. For example, if soft tissue requires higher

**Table 1**  
Scaffold preparation methods with examples (ex).

Preparation method			
Conventional	Ref.	Advanced	Ref.
Solvent casting/particulate leaching (SCPL)	[34]	Electrospinning	[62]
Ex: antibacterial bioactive glass/poly L-lactide composite scaffold.	[35]	-Classical electrospinning	[62]
Melt molding	[51]	Ex: dexamethasone-loaded biphasic calcium phosphate nanoparticles/collagen scaffold.	[67]
Ex: poly (lactic glycolic acid) scaffold.	[52–55]	-Coaxial electrospinning	[73]
Gas foaming		Ex: PLLA/PCL/HA scaffold.	[74]
Ex: polylactic acid scaffold.		Rapid prototyping	[75]
Thermally induced phase separation		- Stereolithography.	
Ex: chitosan/bioactive glass scaffold.		- Selective laser sintering.	[87]
Freeze drying		- Inkjet 3D printer.	
Ex: HEC/alginate/HA scaffolds.		- Multi-inkjet 3D printer	[92]
		Ex: calcium phosphate and collagen scaffolds.	
		-3D bioplotter	
		Ex: Si-hydroxyapatite/poly caprolactone/DMB.	

flexibility, the surface area and interconnected porosity of the scaffold are the target parameters, the electro-spinner technique will be the perfect technique for this application. On other hand, if hard tissue requires a load-bearing material with lesser porosity and high mechanical properties as well as suitable bioactivity, 3D printing or freeze drying of inorganic/organic composites will offer appropriate scaffolds.

### 3. Scaffolds fabrication techniques

The scaffold fabrication techniques coupled with the choice of materials have a vital role in the determining the scaffold properties for the target applications. There are two categories of fabrication, namely, conventional and advanced methods of scaffolds fabrication. Table 1 represents the scaffold fabrication methods, discussed in this review.

#### 3.1. Conventional scaffolds fabrication techniques

##### 3.1.1. Solvent casting/particulate leaching (SCPL)

The solvent casting/particulate leaching (SCPL) is the oldest technique used for scaffolds fabrication. The concept of the method depends on the dispersion of porogens into a polymer solution as shown in Fig. 3. The scaffolds obtained after solidification of the polymer and dissolution of the porogens which left a high volume of pores resulting in a porous scaffold is also known as the foam. Although the simplicity of this technique and its control over the porosity of the fabricated scaffolds through the amount and the size of the porogens are attractive, SCPL lacks the uniform arrangement of salt particles through the polymer solution. This disadvantage is due to the dissimilar density of the salt and the polymer. Another disadvantage is due to the way that polymer and the porogens are mixed where the porogens are enveloped completely by the polymer solution that results in the difficulty of removing salt particles with water. Therefore, the porosity of the scaffolds fabricated by this technique is limited to 90% and the pore sizes range from 5 to 600  $\mu\text{m}$  with irregular microstructures [33,34]. In addition, there are a few additional disadvantages which come typically from the type of the polymer solvent used in which the scaffold material may be solubilized. Typically, organic solvents are utilized, which are frequently lethal, which in turn would prevent the cells seeding onto these scaffolds. Owing to these restrictions of this technique in preparing scaffolds, only a few successful preclinical trials have been demonstrated in mimicking tissues or organ including bone marrow and hard bone regeneration [35,36].

##### 3.1.2. Melt molding

Melt molding technique is based on mixing of gelatin microspheres with a specific polymer powder in a Teflon mold. The mixture is then heated above the polymer glass transition temperature. The best polymer for this method is known to be poly (lactic glycolic acid) (PLGA) due to its lower glass transition temperature. The heating allows the incorporation of bioactive molecules through the gelatin resulted in a structural change which may affect its aqueous solubility. The resulting composite is placed in water after heating in order to dissolve the water-soluble microspheres resulting in a porous structure (Fig. 4). This technique possesses the same disadvantages of the SCPL technique, e.g., the porosity and the pore size depend on the porogen concentration and diameter, respectively. In addition, the variation in scaffold pore sizes is obtained by this technique. On the other hand, in the melt molding technique the use of toxic solvents is avoided [37]. This technique if combined with another one from traditional technique such as particle leaching could be with a potential for tissue regeneration as earlier reported in a preclinical study [38].

##### 3.1.3. Gas foaming

This technique is known as gas foaming technique because it uses a foaming agent (like sodium bicarbonate) into the polymer. High-pressure gas is applied for disks of polymer in order to prompt the nucleation and development of gas rise within the subjected substance (Fig. 5). They are afterwards lyophilized to obtain scaffold characterized with pore diameters of about 100  $\mu\text{m}$  and percentage porosity up to 93% upon the gas liberation (like as  $\text{N}_2$  or  $\text{CO}_2$ ) [39]. Gas is formed due to the action of the acidic aqueous solution with the foaming agent and the liberation of gas producing a porous structure [39]. The disadvantage of this method is that it increases the heterogeneity of the formed foam with a disordered porosity. Here, the top of the foam has a highly porous structure, but the bottom layer exists with a non-porous structure [40–41]. On the other hand, gas foaming procedure is reliable to create solvents-free interconnected network polymeric scaffolds. Some of the prepared scaffolds by this technique were introduced to preclinical stage with stem cells, which showed promising results for bone tissue regeneration [42].

##### 3.1.4. Thermally induced phase separation

This procedure depends on a thermal energy difference that initiates a detachment of a polymer solution with a homogeneous network into a multi-stage system domain using a quench method. In the beginning, a high temperature is utilized to a solubilized polymer (either in phenol or naphthalene), trailed by scattering of naturally dynamic particle in these solutions. Upon the temperature decrease the segregation is prompted, the resulted solution isolates into polymer-free phase and solvent-free phase either by strong fluid de-blending or fluid stage division component. This step is then followed by extraction, dissipation, and sublimation in order to eliminate the used solvent, thus, resulting in 3D polymer matrix impregnated with bioactive particles coordinated within this porous structure. The microstructural characteristics of the achieved scaffolds are adjusted by controlling several factors including the polymer characteristics, solvent, the centralization of the solution of polymer and temperature at which phases are detached. Two kinds of this technique are utilized as shown in Fig. 6, solid-liquid and liquid-liquid separations. The advantage of this method is that it can function with much of other manufacture innovation as well as great mechanical properties obtained for the three-dimensional structures with controlled pore morphology [43,44].

For example, mixing solid naphthalene and poly-lactic acid (PLLA) in a flask, and then heating them with stirring provides a homogenous solution. Afterward, the solution is casted into a cooled mold in order to form polymer-poor and polymer-rich phases. Then, naphthalene is eliminated to produce the porous structure through a vacuum drying stage. The kinetics of the phase separation controls the morphology and pore distribution of the foam. In contrast with the previously mentioned

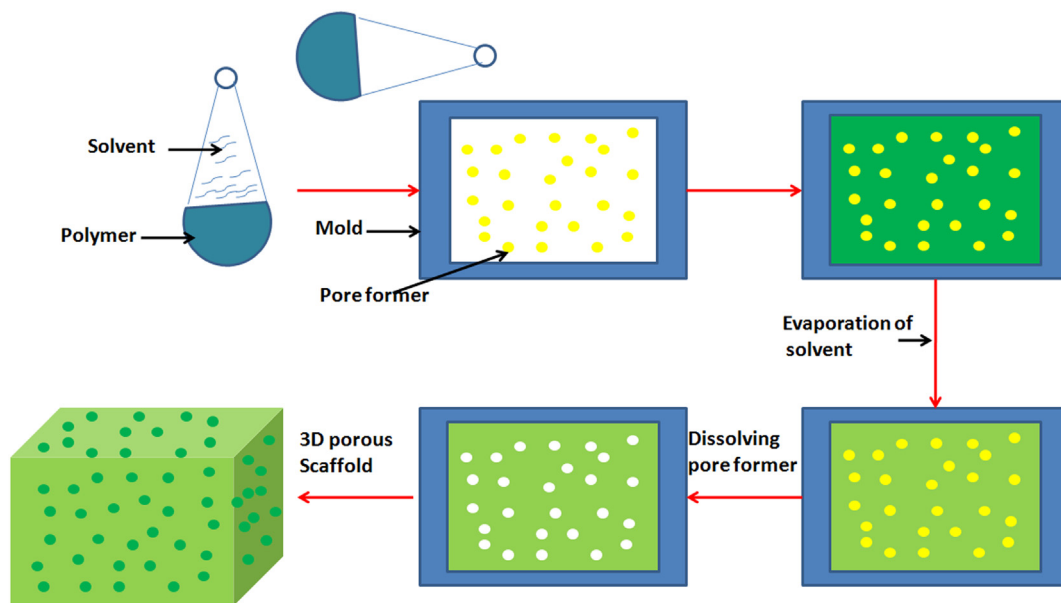


Fig. 3. Demonstration of the solvent casting/particulate leaching (SCPL) technique. Adapted from [33].

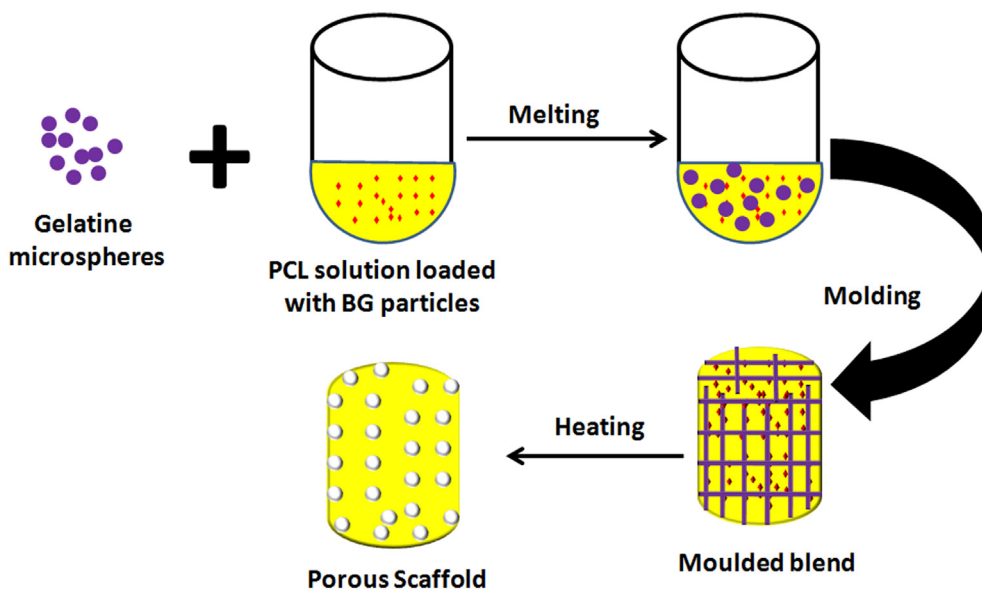


Fig. 4. Schematic illustration showing the melt molding process utilized to fabricate PCL/BG-SA/Gel scaffold. Adapted from [37].

techniques, this technique is characterized by the relative uniformity of the distribution of the pore and the resulting pore diameters range from 50 to 100  $\mu\text{m}$ . The polymer concentration affects the porosity percentage that can reach up to 87%. However, the limitation of this technique rises from the organic solvents usage that might have a toxic effect on cells. There is some evidence of recent study which has used this technique to prepare phase separated nanofibrous vascular scaffolds, modified with heparin and SDF-1 $\alpha$  confirming its applicability as a small diameter vascular graft in the preclinical level [45].

### 3.1.5. Freeze drying technique

All of the above-mentioned techniques have been used in a small number of publications (see Fig. 1a) due to several disadvantages arising from a limited number of applicable materials to those techniques using organic solvent and their lethal effects on cells and non-homogenous microstructure which are not suitable for cells growth.

This was the trend for all of the old techniques except for freeze drying technique. In this technique the porosity of the scaffolds is produced via the lyophilization, where the ice crystals of the solvent are formed after leaving the composite in the freezer are supplemented by using the freeze-drying technique (Fig. 7) [46]. The ice crystals serve as porogens that control the pore sizes and this can be achieved by controlling the freezing temperature and the polymer weight ratio in the solution. This procedure till now has been very beneficial in the design of 3D-frameworks in the room to freeze temperatures and without using organic solvent. It is a lack of dehydration strategy dependent on the evacuation, thus solidified structures are subjected to sublimation process, in which, water particles are evaporated under vacuum, at low pressure, prompting 3D-scaffold in the dried form [47–50]. The porous sponge structure of the produced scaffolds by this technique is preserved even after the immersion in simulated body fluid. Recent trials were conducted using lyophilization technique to prepare various 3D-structures

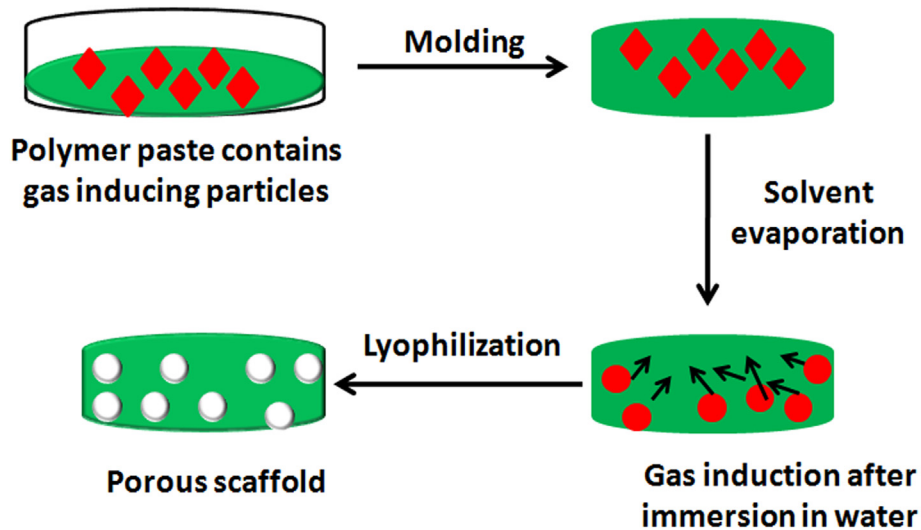


Fig. 5. Scaffold prepared by gas foaming technique. Adapted from [41].

from natural or synthetic polymers and their composite with inorganic biomaterials such as hydroxy apatite and bioactive glass [51–55]. These scaffolds showed promising results when they were tested against normal cells and in vivo in rat models.

### 3.2. Advanced scaffolds fabrication techniques

The conventional strategies for creating 3D-permeable frameworks

in the applications of TE face some serious limitations including difficulties to adjust the microstructure, morphology, connectivity and diameters of the pores as well as the total scaffold porosity. A three-dimensional structure with pore sizes suitable for vascularization of cells become an important need [56]. Therefore, new advanced techniques have arisen, such as electrospinning [57] and rapid prototyping (RP) [58,59]. In the following sections, these advanced strategies will be discussed on several bases including applicability of these systems

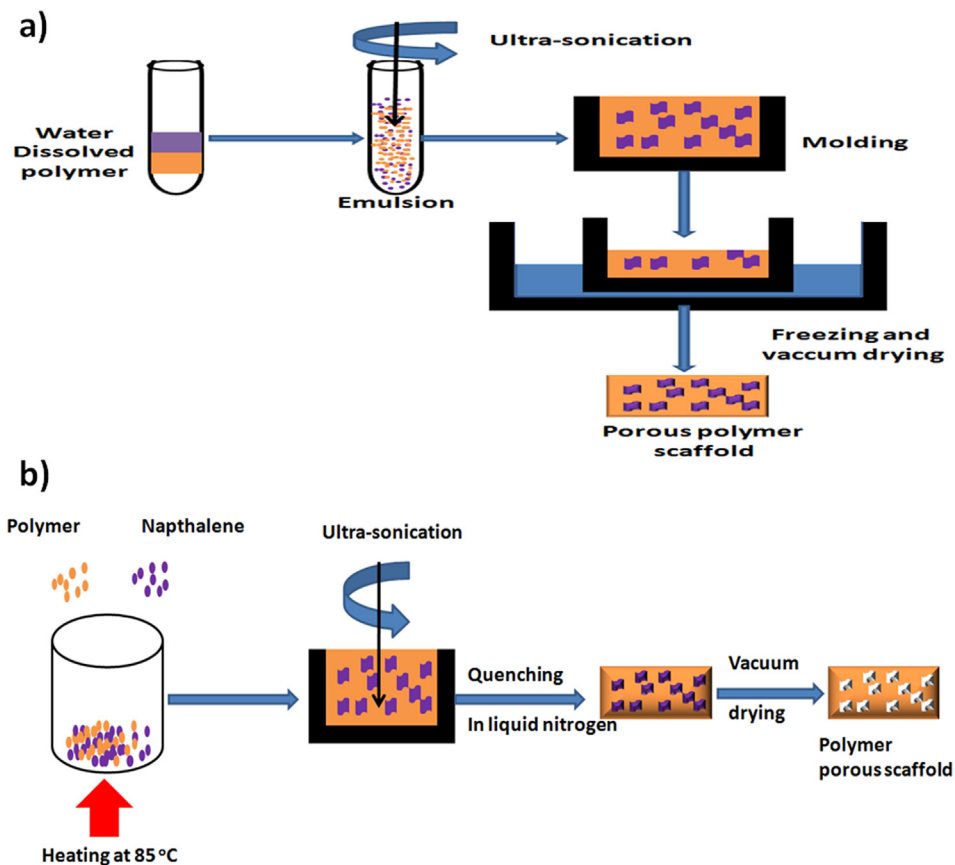


Fig. 6. Schematic diagrams of a) liquid-liquid phase and b) solid-liquid phase separation. Adapted from [44].

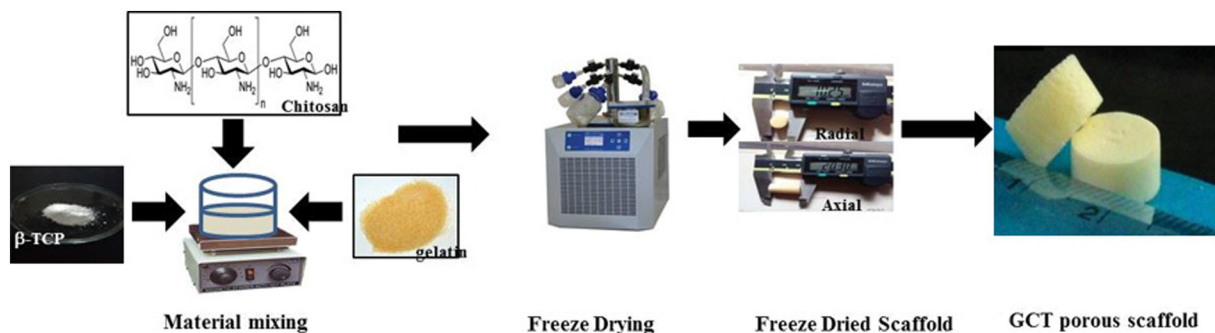


Fig. 7. Scaffold prepared by lyophilization technique [45]. Bioceramics Development and Applications-Open Access Journals.

for TE and the suitability of materials, scaffold development stages and their advantages and restrictions.

### 3.2.1. Electrospinning

Electrospinning strategy is one of the delicate techniques where a 3D-structure is synthesized utilizing electrostatic powers which create fibers from polymer solutions characterized with small fiber diameters in the range of nanometer to micrometer with higher surface area compared to those created by classical spinning forms. Over 200 natural polymers and composites have been utilized in the electrospinning, for example, silk fibroin, chitosan, gelatin, collagen, etc. and plenty of synthetic polymers including (PVA, PVP, PLLA, PCL, etc.) are additionally utilized in this system [60]. To produce the electrospun fibers a high DC voltage ranging between 10 and 40 kV is a must, and this could be done under the ambient conditions.

Electrospinning setups are generally classified into two categories: horizontal and vertical (Fig. 8a). Essentially, an electrospinning setup comprises of three noteworthy parts: a high voltage control supply, a spinneret (e.g., a needle with metal tip) and a metallic collector for the electrospun fibers. In order to prepare a homogeneous solution for electrospinning, the polymers should be ideally dissolved in a carefully selected solvent. Afterwards, the obtained solution is brought into the metal nozzle and subjected to a high voltage source; this in turn accelerates the polymer solutions through the metal tip toward the metal collector of opposite polarity at a steady stream rate [61]. Nevertheless, a few polymers may emanate an undesirable or unsafe smell, so the procedures ought to be led inside closed enclosures with ventilation aperture.

Owing to the use of high voltage in this procedure, the polymer solution is consistently charged, and this causes a repulsive power inside the system [61]. The repulsive electrical powers defeat the surface pressure powers only when the connected electric field reaches a critical value, causing a charged stream of the solution to spout from the tip of the Taylor cone and moves toward the collector charged cathode. Significant favorable circumstances of this system are that it is adaptable, non-obtrusive and temperature independent fibers production method.

It is obvious that this system has recorded an exceptional increment in research and business considerations in various domains within the last ten years as it can provide very suitable substrates for cell growth and consequent tissue development. With the extension of this innovation, a few research teams have grown progressively advanced scaffolds that can create increasingly complicated mats in a progressively controlled and productive way [62,63]. Table 2 summarizes the electrospinning elements, factors controlling fibers diameter and advantage of the electrospinning system for the preparation of scaffolds for TE.

These developments incorporate coaxial electrospinning, in which the spinner fibers are not only one phase of polymer but also could be in a core shell form nanofiber with complicated microstructures, mainly for the production of core shell staggered structures by using more than

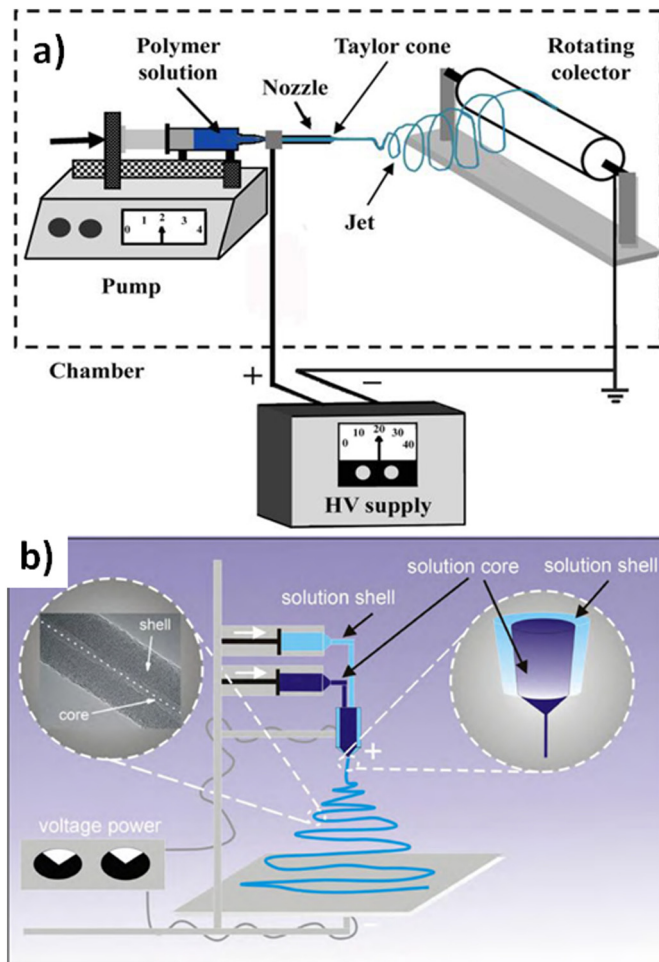


Fig. 8. Different types of electro-spinning a) classical electrospinning reproduced from 6th international conference Bucharest, Romania [70] and b) co-axial electro-spinneret reproduced from PeerJ open access journal [71].

one pump system through coaxial vessels. Thus, this expands the yield production of the fibers and decreases the common electrostatic repulsion in this procedure (Fig. 8b) [64,65]. Numerous parameters influence the fibers microstructural properties, such as, (i) polymer type, the solution viscosity, the polymer solution surface tension, (ii) the pumping rate, the distance between the collector and the needle tip, size of the needle tip, and (iii) the encompassing environment (humidity and temperature) [66].

Impressively, great surface/volume values, adjusted porosity, flexibility to adjust to a wide assortment of sizes and shapes and the capacity to control the nanofiber structure are some of the benefits of the electro-spinning system. The high surface/volume ratios allow the

**Table 2**  
Electrospinning elements, fiber diameter controlling factors and advantages.

Electrospinning elements	Fiber diameter controlling factors	Advantages
High voltage control supply. Extrusion pump connected to syringe with metal tip. Metal collector (stationary or movable)	Polymer concentration and solution viscosity Polymer surface tension Flow rate	An adaptable system for production 3D scaffolds. Suitable for more than 200 natural and synthetic polymers Temperature independent system and suitable for loading of active molecules
Chamber (enclosed system)	Distance between needle tip and collector	High surface to volume ratio

loading of active molecules as well as cell propagation followed by tissue regeneration for the damaged site [67]. Impressive hydrophilicity and biocompatibility properties are obtained which are attributed to the natural polymers specially polysaccharides. Nevertheless, lower mechanical properties are their main disadvantages. If a higher tensile characteristic is the target then the natural polymer-based fibers should be mixed with other synthetic polymers or reinforced by inorganic materials, this in turn would diminish the hydrophobicity of the engineered scaffold [68]. In addition, delivery of active molecules like drugs and growth factors could be enhanced through mixing of various polymers at various proportions [69–71].

Several successful implementations for nanofiber scaffolds in tissue regeneration on both cells and in vivo have been recorded in the literature [62,63,67]. Overall, the electrospinning technology offers great privileges for scientists motivated by TE field, and thus, it demonstrates a large number of suitable polymers, polymer composites and polymer/inorganic composites as fibrous materials. In addition, the flexibility of this technology enables them to adjust the scaffolds microstructural properties, load drugs and bioactive molecules in a way that combines disease treatment with tissue regeneration for the damaged site. This might be the reason behind the increased rates of research publications focused on the implementation of the electrospinning technique (see Fig. 1b) for the synthesis of 3D scaffolds.


### 3.2.2. Rapid prototyping

Rapid prototyping and additive manufacturing, also known as 3D-printing, is a strategy that was first portrayed in the year 1986. The classical name of rapid prototyping strategy is stereolithography (SL) (Fig. 9a) in which thin layers of materials are deposited over each other by hardening the layers utilizing ultraviolet waves [72–74]. Two-photon assimilation by photopolymerization for planning of 3D-structures was initiated from this procedure where blended layers of a photo-initiator agent and a monomer gel are cured and crosslinked by a laser source. The photo-initiator contains two dynamic photons that are activated by a laser light source; thus, the polymerization process takes place [74,75]. Similarity, another strategy was created in particular Selective

Laser Sintering (SLS) (Fig. 9b) to make 3D-structures. SLS utilizes a powerful laser to sinter polymer powders to create 3D-structures [72,76].

In spite of the fact that rapid prototyping is effective in producing 3D-complexes it possesses some genuine impediments. Designers have found that the goals of the printing are course reliant, for example, the 3D-structures delivered utilizing this strategy are observed to be structurally stronger on one side and more fragile on the other side depending upon which side is parallel to the heating from the laser. The second real inconvenience is the warm warpage that arises from the utilization of high temperatures, thus this would restrict the use of biological contents such as proteins and cells owing to their thermo-sensitivity in the manufacture of 3D-structures [77,78]. Not many preclinical trials are recorded for scaffold produced using this technique due to its limitations; however, cell attachment was confirmed for 3D scaffolds from polylactide based polymer printed with the help of this technique [75]. In addition, fused deposition modeling (FDM) [79] was invented that possessed many limitations due to the unavailability of different nozzles with different diameters which in turn led to restricted design of the scaffold architecture. Another rapid prototyping technique that was generally based on solvent-based strategies was developed; however, many limitations in terms of longer fabrication time and weaker mechanical scaffold properties were observed for this technique [80].

Upon the innovation of the first inkjet-based strategy in the year 2000, proteins and endothelial cells were printed within the 3D-structures. For this purpose, the nozzles of a commercial inkjet printer were modified so as to allow the researchers to change the nozzle in the required axial (x-) and lateral (y-) positions. In medication delivery, inkjet printers are most usually implemented via this method. Like the inkjet printers, these printing scaffolds store little beads of the medication on fluid film that exemplify the medication bead to shape microparticles which can be utilized for medication conveyance. As this strategy requires no high temperature, the loading of thermosensitive biomolecules as well as cells was much applicable when compared to the SLS [81,82]. In this technique a head of inkjet printer persistently

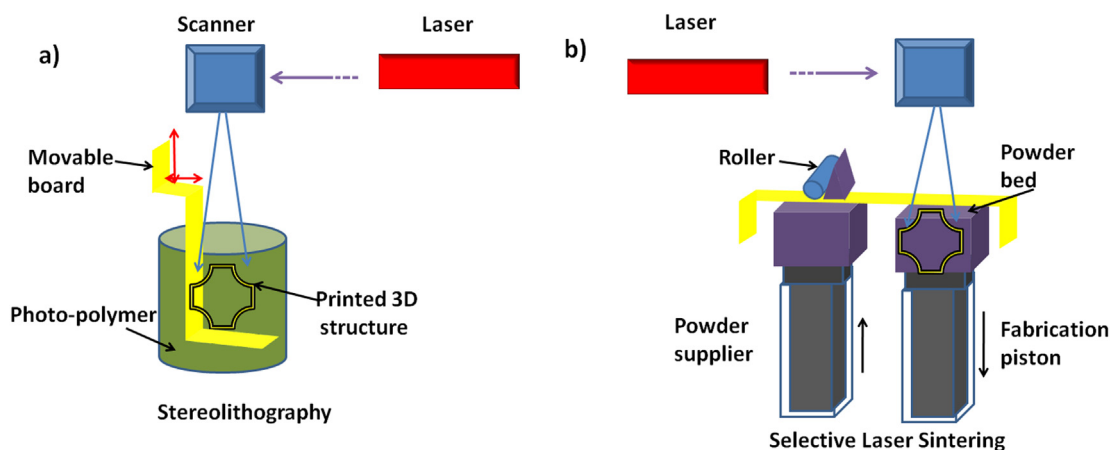

**Fig. 9.** Schematic representation of a) stereolithography (SL) system and b) selective laser sintering (SLS) technique. Adapted from [73].

splashes the medication, cells or other bioactive particles, plus binder onto a bed of polymer powder till a 3D-platform is shaped. In spite of the fact that this method helped in the manufacture of 3D-structures with acceptable mechanical strength, it is not applicable to design of complete 3D-tissue substitutes containing cells or proteins owing to the utilization of binders that in turn diminish the final porosity of the obtained scaffolds [81–84].

Numerous polymers, for example, dextrin, maltodextrin, saccharose and different saps are utilized as binders. These binders normally break down in the dissolvable utilized for bioprinting and after taking back to room temperature, it solidifies, thus resulting in higher compressive bearing for the printed polymer and/or polymer composite scaffolds. These binders are sugar derivative polymers that can be effectively degraded in the circulatory systems to give glucose [84–86]. Poly-saccharide polymers were decomposed to carbon upon applying of relative high temperatures [87,88]. Polymers, for example, teflon (poly-tetrafluoroethylene) and polypropylene may likewise be utilized as binders alongside natural or semi-manufactured materials. For example, collagen as they give enhanced compressive strength to the 3D-structures and furthermore assistance in avoiding corruption and maintaining of the platform while utilizing acidic solvents. Presence of such binders in the printed 3D-structures results in semi-porosity-free. Furthermore, the pore diameters of the platform cannot be adjusted through the printing process and this count as a drawback for the inkjet printing [89]. Low volume launch of ultrasound waves onto the deposition medium followed by ejection of an acoustic droplet (Fig. 10) are initiated from inkjet printing [90–93].

In vivo experiments were conducted with numerous 3D-printed polymeric and ceramic structures in order to evaluate their ability for cytocompatibility and recovery. HAp/PCL and demineralized bone scaffolds substituted with silicon were designed employing rapid prototyping instrument. They possessed abilities for great osseointegration, osteoinductivity and bone recovery when applied to rabbit models [94,95]. Also, an improved bone recovery in rat models was confirmed for 3D-structures made of resorbable dicalcium phosphate (DCP) and prepared utilizing the SLS technique [95]. DCP 3D-structures obtained with different techniques of additive manufacturing (e.g., tank polymerization, powder bed fusion, material extrusion, and binder streaming additionally), which have demonstrated osteogenic potential on the in vitro basis, however, they should be further approved utilizing in vivo examinations [96]. Silicate and phosphate families 3D-printed

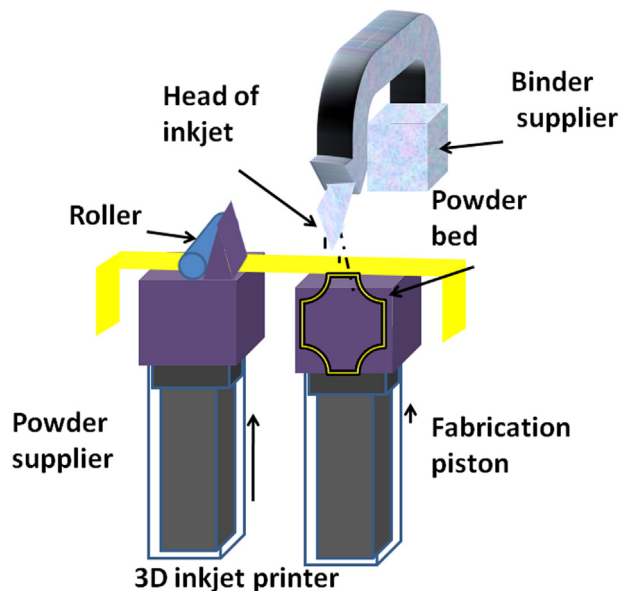


Fig. 10. Scheme demonstrates acoustic droplet ejection 3D printing process. Adapted from [73].

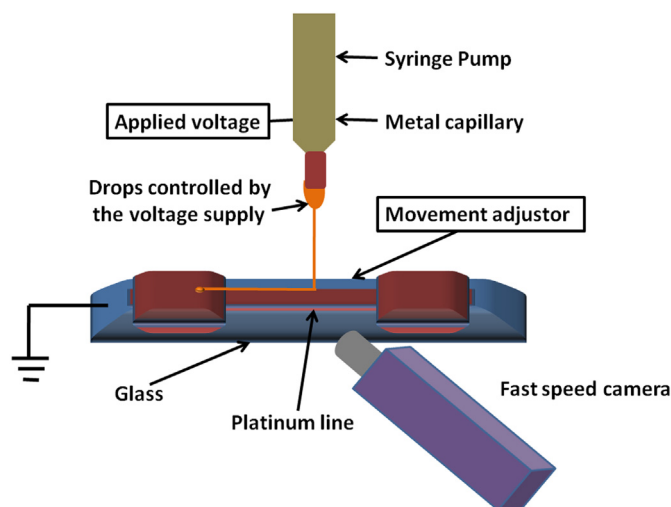


Fig. 11. Schematic diagram of advanced version of 3D-bioprinter which controls the polymer printing rate using voltage supply. Adapted from [109].

scaffolds showed great success in the recovery of bone defects, especially when they are complied with DNA [97].

For tissue recovery, the most preferred biomaterials are hydrogels owing to their customizable hydrating capacity and mechanical characteristics, thus, enabling them to mimic the natural tissue. PEG, gelatin and fibrin hydrogels as well as their derivatives were the most common hydrogels utilized from natural and synthetic polymers in 3D printing loaded with cells for bone recovery applications. Extrusion technique seems to be the most well-known strategy utilized for cell-loaded hydrogel blends [98,99]. In this case, a syringe pump loaded with the solvent moves in the z-axis is utilized and the printing stage moves along the y-axis for the cell-based printing [98]. Applying voltage on the inkjet head can assist in controlling the speed of the solvent splashing and solvent droplet speed can be adjusted by applying differential voltage as shown in Fig. 11 [99]. The correct choice and optimization of these factors are very essential in the 3D printing procedure as they decide the pore size and homogeneity of the 3D-structures [99–101]. Engineered polymers and hydrogels originated from PCL and PLGA are very common in producing of 3D-frameworks utilizing rapid prototyping, have demonstrated great recovery for rabbit tibias bone [99].

However, many restrictions are originated from the 3D printed techniques and this might be the reason behind the decrease in the number of the publications recorded for scaffold synthesis by 3D printing technique when compared to those produced by the electro-spinning technique. These restrictions are represented in limited precursor materials that are applicable for the 3D printing technology, long time for optimization of the design parameters as well as preserving the cell viability during and after the printing. All of these reasons were enough to hold back the progress of the 3D printing technique; however, a lot of work is conducted right now in this regard which might result in the change of this rate. Nowadays, researches are conducted to advance materials to prepare platforms according to the patient-needs for bone recovery utilizing the computerized tomography (CT) scan of patient to print big hard tissue replacers. Utilizing open source coding programming, the CT scans are extrapolated, and 3D printed to shape the bone substitutions that are anatomically like the scan with comparable microstructural properties. The platform could then be covered or loaded up with the undifferentiated cells from the patient and embedded again into the patient's body, consequently enhancing bone recovery and disposing of any opportunity of dismissal [102–108]. Presently, the 3D-printed polymer platforms are being evaluated and directed for use as viable medication delivery frameworks and tissue



substitutes in the field of medical procedure and medicine utilizing natural polymers, for example, chitosan and alginate.

#### 4. Tissue and organ printing

Recreating the perplexing inward vascular system of organs, instead of the assembling procedure itself is the greatest difficulty facing the scientists' desire to print tissues or organs. Subsequently, numerous scientists have directed their concentration to the printing of vein 3D-structures. Vascular prostheses were delivered for the first time in 2009 by Ganovo in the United States where they employed 3D printing [110]. Agarose/cells mixture was employed as cells support in order to obtain vein 3D-structure with diameter of 3 mm by the Southern California University of Health Sciences [111]. Manufacturing of complicated living structures with coordinated micro-vessels utilizing multiple print heads and extraordinary "ink" were revealed by researchers from the Wyss Institute for Biologically Inspired Engineering, Harvard University [107]. Amid the manufacture of tissue incorporated with veins, different kinds of cells, and extracellular framework, a 3D bioprinter with a few freely controlled print heads was planned to develop these heterogeneous 3D-structures with various materials. These scaffolds constituents should be printed exactly with the same characteristics and at the same time. Gelatin methacrylate (GelMA) is utilized as a cell support matrix, while poly (dimethyl siloxane) (PDMS) pigmented with various fluorophores is utilized to label distinctive biomaterials [112].

Complete cellularized skin substitute loaded with fibroblasts and keratinocytes in a typical 3D spatial model was produced by using bioprinting associated with laser aid [113], where, comprising of fibroblasts labeled in red and keratinocytes labeled in green on the surface of MatriDerm®, that was used to treat skin wound in the mouse. Untreated part of the mouse skin was used as a negative control for comparison. After testing the skin builds by utilizing the dorsal skin overlay chamber in naked mice, the printed cells stayed dynamic, kept multiplying, and generated the ECM. A bioprinting procedure for various layers of cells is an essential for making complex tissue with bigger size. Mannoor et al. [114] utilized hydrogel loaded with chondrocyte cells to print a bionic ear. In addition, in the anatomic geometry of a human ear and cochlea-formed terminals silver nanoparticles were loaded (Fig. 12(a,b)). The printed bionic ear is recommended to be utilized as a sound-related detecting device of radio frequencies than the human ear. Working cardiovascular valve was introduced by a scientist from Cornell University which used undeveloped cells and biopolymer materials (Fig. 12(c)), and the loaded cells were transformed bit by bit into mature cells.

It is worthy to highlight that 3D printed organs for clinical applications are presently available. For example, the world's first effective 3D printed transplantation of human organ was done by Michigan University, where they had implanted a synthetic trachea into the windpipe of a baby with a birth deformity to help develop baby's breathing and speech (Fig. 12(d)). Other successful trials for the 3D bioprinting of tissue or organs were reported for several damaged sites at the preclinical stage, among those trails the orthopedic tissue regenerations for different sites such as cartilage [115], complete tooth [116], tooth root and support [117]. Soft tissues printing trials were also reported for skin [118] and few other internal organs, such as, nerve [119], tendon [120], ligament [121], and heart [122].

#### 5. 3D printing restrictions

The utilization of 3D printing innovation for restorative implementations will unravel the contributor deficiency issue for organ transplantations. In this way a rising and quickly created interdisciplinary field will develop that firmly incorporates science of material, cell biology, and clinical science. In spite of the fact that cell loading in 3D structure is possible, considerable work still needs to be conducted to accomplish the perfect mimicry of the original tissue

[123]. It is hard to mimic the structure and organ capacity of the ECM in vitro, as it is a complicated framework with different constituents. This issue is overcome by the consolidation of conciliatory material during the development of a platform. This material gives mechanical help to printing material by occupying the void spaces. These materials are expelled by post preparing after the creation. Impediment initiated by the structure cause brokenness of material due to the poor productivity of CAD plan into the machine [124]. Existing innovations that fundamentally utilize hydrogels loaded with cells cannot resolve the issues of cell nourishment and supplying of oxygen. For bigger scaffolds, an adequate number of cells cannot be supplied at present. Contrasted with cells that adhere to the scaffold outer surface, pre-prophase cells do not get a satisfactory supply of supplements. This leads to non-homogenous distribution to the cells within the 3D matrix [125]. Additionally, different restrictions that incorporate cell survival, advancement, separation, and propagation, should be illuminated for the further improvement of 3D structures printed, tissues, and organs.

Materials confinements likewise occur based on the inherent properties of utilized materials. A significant number of the metal materials that are commonly utilized for permanent implants have a high flexible modulus, which frequently prompts a versatile mismatch between the surrounding environments and implant. Printed biodegradable 3D structures are commonly created from characteristic polymers with great biocompatibility, however, they possess low mechanical strength, for example, sodium alginate, collagen, and different hydrogels. Moreover, there are no global measures for picking biomaterials for 3D scaffolds. Hence, just engineered assessments can be made depending on structure, work, clinical impacts, and different features, instead of assessments dependent on solid markers and adequate exploratory proof. Nowadays, scientists have developed autonomous research and basic systems, which have mostly constrained the improvement of this innovation for medical applications. In addition, ethical issues and cells stimulation are necessary to be considered. In this manner, accomplishing the real usage of 3D printing for restorative applications will require prolonged range endeavors [126–128].

#### 6. Conclusions

After exploring the conducted research work related to the tissue regeneration applications, it was confirmed that TE could be considered as one of the chosen ways to deal with the ordinary tissue regeneration problems, based on both laboratory and preclinical studies but not yet on the basis of clinical trials. The production of scaffold as the essential subunit that supports mechanical properties, cell adhering, proliferation, and specialization, could be achieved by manipulating the major key factors like material choice and 3D-structure creation method that are suitable for specific organ damage or defect. Though the use of some traditional techniques on both lab and preclinical bases (freeze drying) still apply for this purpose when one compares it with advanced techniques, the demands for sophisticated TE field hold great promises for the advanced techniques as could be noted from literature. Electrospinning technique is of interest for the production of 3D scaffolds owing to its tunable parameters and, thus, it has grown fast in both industrial and biomedical fields. On the other hand, 3D printing possesses slow evolution rate when it is compared to the electrospinning technique as it is a complicated process with multiple engineering factors with no respect to the biological systems. Therefore, in the current days, much advancement was considered to develop the 3D printer system in a compatible manner with tissue and organ conditions. Accordingly, both electrospinning and 3D printing technologies are guiding the ways for scientists to develop 3D-structures with cutting edge methods utilizing diverse range of biomaterials which are now their focal point of research endeavors in the field of TE.

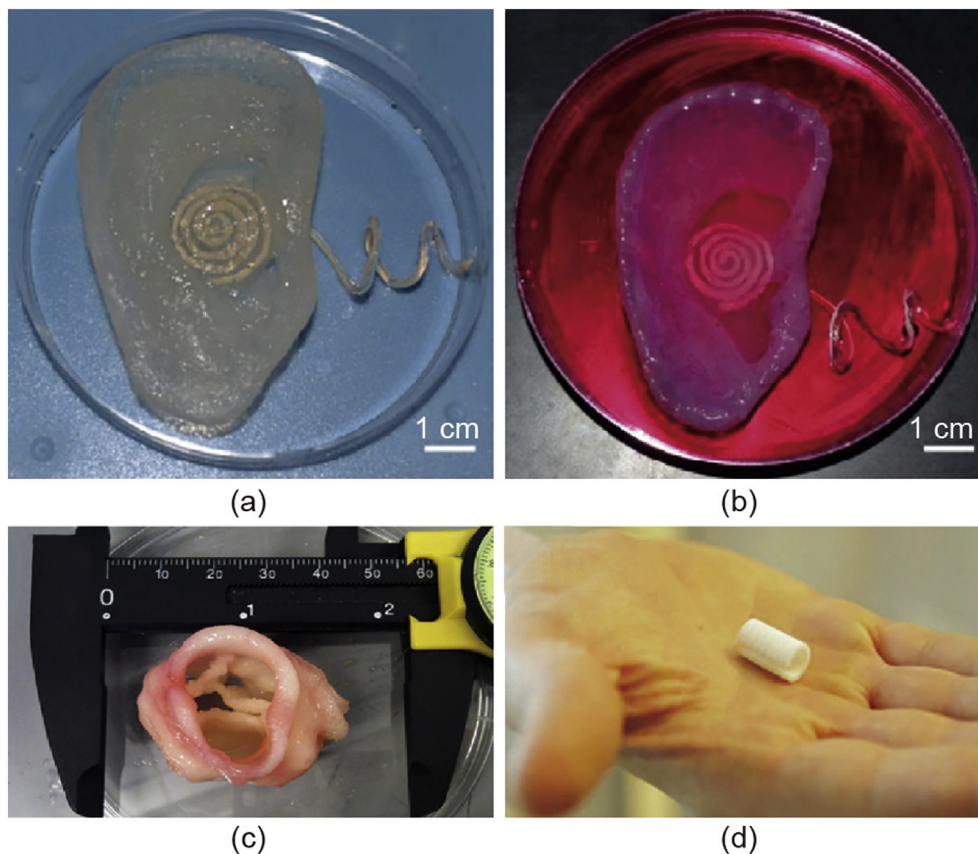


Fig. 12. Illustrations for (a) bionic ear upon 3D printing; (b) bionic ear during in vitro culturing; (c) cardiac valve and (d) artificial trachea [114].

### Declaration of competing interest

None.

### Acknowledgment

The authors wish to express their sincere appreciation to the Academy of Medical Sciences, London, UK for supporting financially an academic visit of Dr. Mostafa Mabrouk to Loughborough University through a Daniel Turnberg UK/Middle East Travel Fellowship.

### References

- [1] S. Giwa, J.K. Lewis, L. Alvarez, et al., The promise of organ and tissue preservation to transform medicine, *Nat. Biotechnol.* 35 (6) (2017) 530–542.
- [2] B. Jones, M. Bes, Keeping kidneys, *Bull. World Health Organ.* 90 (10) (2012) 718–719.
- [3] M. Colvin, J.M. Smith, M.A. Skeans, et al., OPTN/SRTR 2015 annual data report: heart, *Am. J. Transplant.* 17 (1) (2017) 286–356.
- [4] A. Hart, J.M. Smith, M.A. Skeans, et al., OPTN/SRTR 2015 annual data report: kidney, *Am. J. Transplant.* 17 (1) (2017) 21–116.
- [5] A.K. Israni, D. Zaun, C. Bolch, et al., OPTN/SRTR 2015 annual data report: deceased organ donation, *Am. J. Transplant.* 17 (1) (2017) 503–542.
- [6] B.L. Kasiske, S.K. Asrani, M.A. Dew, et al., The living donor collective: a scientific registry for living donors, *Am. J. Transplant.* 17 (12) (2017) 3040–3048.
- [7] S. Nagral, M. Hussain, S.A. Nayeem, R. Dias, S.A. Enam, S. Nundy, Unmet need for surgery in south asia, *BMJ* 357 (2017) (article j1423).
- [8] A.M. Bailey, M. Mendicino, P. Au, An FDA perspective on preclinical development of cell-based regenerative medicine products, *Nat. Biotechnol.* 32 (8) (2014) 721–723.
- [9] P.S. Knoepfler, From bench to FDA to bedside: us regulatory trends for new stem cell therapies, *Adv. Drug Deliv. Rev.* 82–83 (2015) 192–196.
- [10] X.L. Tang, Q. Li, G. Rokosh, et al., Long-term outcome of administration of c-kitPOS cardiac progenitor cells after acute myocardial infarction: transplanted cells do not become cardiomyocytes, but structural and functional improvement and proliferation of endogenous cells persist for at least one year, *Circ. Res.* 118 (7) (2016) 1091–1105.
- [11] S. Bose, M. Roy, A. Bandyopadhyay, Recent advances in bone tissue engineering scaffolds, *Trends Biotechnol.* 30 (10) (2012) 546–554.
- [12] L.L. Hench, The future of bioactive ceramics, *J. Mater. Sci. Mater. Med.* 26 (2) (2015) 86.
- [13] R. Detsch, S. Alles, J. Hum, P. Westenberger, F. Sieker, D. Heusinger, A.R. Boccaccini, Osteogenic differentiation of umbilical cord and adipose derived stem cells onto highly porous 45S5 Bioglass®-based scaffolds, *J. Biomed. Mater. Res. A* 103 (3) (2015) 1029–1037.
- [14] R. El-Gendy, J. Kirkham, P.J. Newby, Y. Mohanram, A.R. Boccaccini, X.B. Yang, Investigating the vascularization of tissue-engineered bone constructs using dental pulp cells and 45S5 Bioglass® scaffolds, *Tissue Eng. A* 21 (13–14) (2015) 2034–2043.
- [15] A. Philippart, A.R. Boccaccini, C. Fleck, D.W. Schubert, J.A. Roether, Toughening and functionalization of bioactive ceramic and glass bone scaffolds by biopolymer coatings and infiltration: a review of the last 5 years, *Expert review of medical devices* 12 (1) (2015) 93–111.
- [16] T. Dvir, B.P. Timko, D.S. Kohane, R. Langer, Nanotechnological strategies for engineering complex tissues, *Nat. Nanotechnol.* 6 (1) (2011) 13.
- [17] G. Gao, X. Cui, Three-dimensional bioprinting in tissue engineering and regenerative medicine, *Biotechnol. Lett.* 38 (2) (2016) 203–211.
- [18] X. Guan, M. Avci-Adali, E. Alarcin, et al., Development of hydrogels for regenerative engineering, *Biotechnol. J.* 12 (5) (2017) 1–19.
- [19] M.J. Kraeutler, J.W. Belk, J.M. Purcell, E.C. McCarty, Microfracture versus autologous chondrocyte implantation for articular cartilage lesions in the knee: a systematic review of 5-year outcomes, *Am. J. Sports Med.* 46 (4) (2017) 995–999.
- [20] H. Mistry, M. Connock, J. Pink, et al., Autologous chondrocyte implantation in the knee: systematic review and economic evaluation, *Health Technol. Assess.* 21 (6) (2017) 1–294.
- [21] A.G. Guex, F.M. Kocher, G. Fortunato, et al., Fine-tuning of substrate architecture and surface chemistry promotes muscle tissue development, *Acta Biomater.* 8 (4) (2012) 1481–1489.
- [22] A.S. Mao, D.J. Mooney, Regenerative medicine: current therapies and future directions, *Proc. Natl. Acad. Sci. U. S. A.* 112 (47) (2015) 14452–14459.
- [23] M. Alves da Silva, A. Martins, A.R. Costa-Pinto, et al., Electrospun nanofibrous meshes cultured with Wharton's jelly stem cell: an alternative for cartilage regeneration, without the need of growth factors, *Biotechnol. J.* 12 (12) (2017) 1–9.
- [24] A.I. Goncalves, M.T. Rodrigues, M.E. Gomes, Tissue engineered magnetic cell sheet patches for advanced strategies in tendon regeneration, *Acta Biomater.* 63 (2017) 110–122.
- [25] S. Pina, R.F. Canadas, G. Jimenez, et al., Biofunctional ionic doped calcium phosphates: silk fibroin composites for bone tissue engineering scaffolding, *Cells Tissues Organs* 204 (3–4) (2017) 150–163.
- [26] L. Drowley, C. Koonce, S. Peel, et al., Human induced pluripotent stem cell-derived

- cardiac progenitor cells in phenotypic screening: a transforming growth factor- $\beta$  type 1 receptor kinase inhibitor induces efficient cardiac differentiation, *Stem Cells Transl. Med.* 5 (2) (2016) 164–174.
- [27] K. Dzubo, T. Turnley, A. Wishart, et al., Fibroblast-derived extracellular matrix induces chondrogenic differentiation in human adipose-derived mesenchymal stromal/stem cells in vitro, *Int. J. Mol. Sci.* 17 (8) (2016) 1–20.
- [28] N.D. Evans, E. Gentleman, X. Chen, C.J. Roberts, J.M. Polak, M.M. Stevens, Extracellular matrix-mediated osteogenic differentiation of murine embryonic stem cells, *Biomaterials* 31 (12) (2010) 3244–3252.
- [29] K. Sadtler, A. Singh, M.T. Wolf, X. Wang, D.M. Pardoll, J.H. Elisseeff, Design, clinical translation and immunological response of biomaterials in regenerative medicine, *Nat. Rev. Mater.* 1 (7) (2016) 201616040.
- [30] A. Atala, Regenerative medicine strategies, *Journal of Pediatric Surgery* 47 (1) (2012) 17–28.
- [31] D.N. Kotton, E.E. Morrissey, Lung regeneration: mechanisms, applications and emerging stem cell populations, *Nat. Med.* 20 (8) (2014) 822–832.
- [32] S.G. Kumbhar, S.H. Pawar, Self-functionalized, oppositely charged chitosan-alginate scaffolds for biomedical applications, *Biotechnol. Bioeng.* 113 (2) (2017) 130.
- [33] D. Bartis, J. Pongracz, *Three Dimensional Tissue Cultures and Tissue Engineering*, (2011), <https://doi.org/10.13140/2.1.2793.5047>.
- [34] A.M. El-Kady, R.A. Rizk, B.M. Abd El-Hady, M.W. Shafaa, M.M. Ahmed, Characterization, and antibacterial properties of novel silver releasing nano-composite scaffolds fabricated by the gas foaming/salt-leaching technique, *Journal of Genetic Engineering and Biotechnology* 10 (2012) 229–238.
- [35] A. Sola, J. Bertacchini, D. D'Avella, et al., Development of solvent-casting particulate leaching (SCPL) polymer scaffolds as improved three-dimensional supports to mimic the bone marrow niche, *Mater. Sci. Eng. C* 96 (2019) 153–165.
- [36] Y. Xie, X.-R. Lan, R.-Y. Bao, et al., High-performance porous polylactide stereo-complex crystallite scaffolds prepared by solution blending and salt leaching, *Mater. Sci. Eng. C* 90 (2018) 602–609.
- [37] D. Mao, Q. Li, D. Li, Y. Tan, Q. Che, 3D porous poly( $\epsilon$ -caprolactone)/58S bioactive glass–sodium alginate/gelatin hybrid scaffolds prepared by a modified melt molding method for bone tissue engineering, *Mater. Des.* 160 (2018) 1–8.
- [38] H.-M. Yin, J. Qian, J. Zhang, Engineering porous poly(lactic acid) scaffolds with high mechanical performance via a solid state extrusion/porogen leaching approach, *Polymers* 8 (2016) 213, <https://doi.org/10.3390/polym8060213>.
- [39] S.P. Soundarya, A.H. Menon, S.V. Chandran, N. Selvamurugan, Bone tissue engineering: scaffold preparation using chitosan and other biomaterials with different design and fabrication techniques, *Int. J. Biol. Macromol.* 119 (2018) 1228–1239.
- [40] X. Liao, H. Zhang, T. He, Preparation of porous biodegradable polymer and its nanocomposites by supercritical CO<sub>2</sub> foaming for tissue engineering, *J. Nanomater.* 6 (2012) 1–12.
- [41] X. Wang, W. Li, V. Kumar, A method for solvent-free fabrication of porous polymer using solid-state foaming and ultrasound for tissue engineering applications, *Biomaterials* 27 (9) (2006) 1924–1929.
- [42] C. Ceccaldi, R. Bushkalova, D. Cussac, et al., Elaboration and evaluation of alginate foam scaffolds for soft tissue engineering, *Int. J. Pharm.* 524 (1–2) (2017) 433–442.
- [43] G. Tarun, S. Onkar, A. Saahil, R. Murthy, Scaffold: a novel carrier for cell and drug delivery, *Crit. Rev. Ther. Drug Carrier Syst.* 29 (2012) 1–63, <https://doi.org/10.1615/CritRevTherDrugCarrierSyst.29> (10).
- [44] U.G. Sampath, Y.C. Ching, C.H. Chuah, J.J. Sabariah, P.C. Lin, Fabrication of porous materials from natural/synthetic biopolymers and their composites, *Materials* 9 (12) (2016) 991.
- [45] W. Wang, D. Liu, D. Li, et al., Nanofibrous vascular scaffold prepared from miscible polymer blend with heparin/stromal cell-derived factor-1 alpha for enhancing anticoagulation and endothelialization, *Colloids Surf. B: Biointerfaces* 181 (2019) 963–972.
- [46] C.A. Martínez-Pérez, I. Olivas-Armendariz, J.S. Castro-Carmona, P.E. García-Casillas, Scaffolds for tissue engineering via thermally induced phase separation, *Advances in Regenerative Medicine*, InTech, 2011.
- [47] H. Liu, T. Webster, *Bioinspired Nanocomposites for Orthopedic Applications*, (2007), [https://doi.org/10.1142/9789812779656\\_0001](https://doi.org/10.1142/9789812779656_0001).
- [48] A.S. Siva, M.N.M. Ansari, A review on bone scaffold fabrication methods, *Int. Res. J. Eng. Technol.* 2 (6) (2015) 1232–1237.
- [49] M. Brotto, M.L. Johnson, Endocrine crosstalk between muscle and bone, *Curr. Osteoporos. Rep.* 12 (2) (2014) 135–141.
- [50] K. Maji, S. Dasgupta, Effect of  $\beta$ -tricalcium phosphate nanoparticles additions on the properties of gelatin-chitosan scaffolds, *Bioceram. Dev. Appl.* 7 (103) (2017), <https://doi.org/10.4172/2090-5025.1000103>.
- [51] S. Boullila, H. Oudadesse, R. Kallel, B. Lefevre, M. Mabrouk, K. Chaabouni, F.M. Ayedi, T. Boudawara, A. Elfeki, H. Elfeki, In vivo study of hybrid biomaterial scaffold bioactive glass–chitosan after incorporation of Ciprofloxacin, *Polym. Bull.* 74 (10) (2017) 4153–4173, <https://doi.org/10.1007/s00289-017-1936-z>.
- [52] R.V. Badhe, D. Bijukumar, D.R. Chejara, M. Mabrouk, Y.E. Choonara, P. Kumar, L.C. du Toit, P.P.D. Kondiah, V. Pillay, A composite chitosan-gelatin bi-layered, biomimetic macroporous scaffold for blood vessel tissue engineering, *Carbohydr. Polym.* 157 (2017) 1215–1225.
- [53] K.M. Tohamy, M. Mabrouk, I.E. Soliman, H.H. Beherei, M.A. Aboelnasr, Novel alginate/hydroxyethyl cellulose/hydroxyapatite composite scaffold for bone regeneration: in vitro cell viability and proliferation of human mesenchymal stem cells, *Int. J. Biol. Macromol.* 112 (2018) 448–460.
- [54] E. El-Meliigy, M. Mabrouk, S.A.M. El-Sayed, B.M. Abd El-Hady, M.R. Shehata, Wafaa M. Hosny, Novel Fe<sub>2</sub>O<sub>3</sub>-doped glass/chitosan scaffolds for bone tissue replacement, *Ceram. Int.* 44 (2018) 9140–9151.
- [55] K.M. Tohamy, I.E. Soliman, M. Mabrouk, S. ElShebiney, H.H. Beherei, M.A. Aboelnasr, D.B. Das, Novel polysaccharide hybrid scaffold loaded with hydroxyapatite: fabrication, bioactivity, and in vivo study, *Materials Science & Engineering C* 93 (2018) 1–11.
- [56] J. Zhang, S. Zhao, M. Zhu, Y. Zhu, Y. Zhang, Z. Liu, C. Zhang, 3D-printed magnetic Fe<sub>3</sub>O<sub>4</sub>/MBG/PCL composite scaffolds with multifunctionality of bone regeneration, local anticancer drug delivery and hyperthermia, *J. Mater. Chem. B* 2 (2014) 7583.
- [57] D.K. Srinivasan, C. Gandhimathi, J.R. Venugopal, S. Ramakrishna, S.S.W. Tay, Osteogenic potency of electrosprayed silk fibroin/hydroxyapatite nanoparticles—an innovative approach for bone tissue engineering, *FASEB J.* 30 (2016).
- [58] T.K. Merceron, M. Burt, Y.-J. Seol, H.-W. Kang, S.J. Lee, J.J. Yoo, A. Atala, A 3D bioprinted complex structure for engineering the muscle–tendon unit, *Biofabrication* 7 (2015) 035003.
- [59] A. Abarrategi, C. Moreno-Vicente, F.J. Martínez-Vázquez, A. Civantos, V. Ramos, J.V. Sanz-Casado, R. Martínez-Corria, F.H. Perera, F. Mulero, P. Miranda, J.L. López-Lacomba, Biological properties of solid free form designed ceramic scaffolds with BMP-2: in vitro and in vivo evaluation, *PLoS One* 7 (3) (2012) e34117.
- [60] T.J. Sill, H.A. von Recum, T.J. Sill, H.A. von Recum, Electrospinning: applications in drug delivery and tissue engineering, *Biomaterials* 29 (13) (2008) 1989–2006. Electrospinning: applications in drug delivery and tissue engineering, *Biomaterials* 29 (13) (2008) 1989–2006.
- [61] Z.M. Huang, Y.Z. Zhang, M. Kotaki, S. Ramakrishna, A review on polymer nanofibers by electrospinning and their applications in nanocomposites, *Compos. Sci. Technol.* 63 (15) (2003) 2223–2253.
- [62] Y. Chen, N. Kawazoe, G. Chen, Preparation of dexamethasone-loaded biphasic calcium phosphate nanoparticles/collagen porous composite scaffolds for bone tissue engineering, *Acta Biomater.* 67 (2017) 341–353.
- [63] Y. Lei, Z. Xu, Q. Ke, W. Yin, Y. Chen, C. Zhang, Y. Guo, Strontium hydroxyapatite/chitosan nanohybrid scaffolds with enhanced osteoinductivity for bone tissue engineering, *Mater. Sci. Eng. C* 72 (2017) 134–142.
- [64] X. Qin, *Coaxial Electrospinning of Nanofibers*, *Electrospun Nanofibers*, (2017), pp. 41–71.
- [65] M. Wojasiński, J. Goławski, T. Ciach, Blow-assisted multi-jet electrospinning of poly-L-lactic acid nanofibers, *J. Polym. Res.* 24 (5) (2017) 76.
- [66] W. Cui, Y. Zhou, J. Chang, Electrospun nanofibrous materials for tissue engineering and drug delivery, *Sci. Technol. Adv. Mater.* 11 (1) (2010) 014108.
- [67] H. Qi, Z. Ye, H. Ren, N. Chen, Q. Zeng, X. Wu, T. Lu, Bioactivity assessment of PLLA/PCL/HAP electrospun nanofibrous scaffolds for bone tissue engineering, *Life Sci.* 148 (2016) 139–144.
- [68] H. Liu, X. Ding, G. Zhou, P. Li, X. Wei, Y. Fan, Electrospinning of nanofibers for tissue engineering applications, *J. Nanomater.* 3 (2013) (2013).
- [69] S. Bose, S. Tarafder, Calcium phosphate ceramic systems in growth factor and drug delivery for bone tissue engineering: a review, *Acta Biomater.* 8 (4) (2012) 1401–1421.
- [70] A. Rabbi, K. Nasouri, S.A. Mousavi, A. Haji, Fabrication of Electrospun Polyacrylonitrile and Polyurethane Nanofibers for Sound 6th International Conference Bucharest, Romania, October, (2013), pp. 17–18.
- [71] Hudecki, et al., Structure and properties of slow-resorbing nanofibers obtained by (co-axial) electrospinning as tissue scaffolds in regenerative medicine, 2017, *PeerJ* 5 (2017), <https://doi.org/10.7717/peerj.4125> e4125.
- [72] B.C. Gross, J.L. Erkal, S.Y. Lockwood, C. Chen, D.M. Spence, Evaluation of 3D printing and its potential impact on biotechnology and the chemical sciences, *Anal. Chem.* 89 (7) (2014) 3240–3253.
- [73] S.M. Peltola, F.P. Melchels, D.W. Grijpma, M. Kellomäki, A review of rapid prototyping techniques for tissue engineering purposes, *Ann. Med.* 40 (4) (2008) 268–280.
- [74] S.V. Murphy, A. Atala, 3D bioprinting of tissues and organs, *Nat. Biotechnol.* 32 (8) (2014) 773.
- [75] A. Selimis, V. Mironov, M. Farsari, Direct laser writing: principles and materials for scaffold 3D printing, *Microelectron. Eng.* 132 (2015) 83–89.
- [76] B. Mueller, Additive manufacturing technologies—rapid prototyping to direct digital manufacturing, *Assem. Autom.* 32 (2) (2012).
- [77] S. Kumar, Selective laser sintering: a qualitative and objective approach, *JOM* 55 (10) (2003) 43–47.
- [78] . C.R. Deckard, J.J. Beaman, J.F. Darrah, U.S. Patent No. 5,155,324, U.S. Patent and Trademark Office, Washington, DC, (1992).
- [79] I. Zein, et al., Fused deposition modeling of novel scaffold architectures for tissue engineering applications, *Biomaterials* 23 (4) (2002) 1169–1185.
- [80] D.B. Kolesky, et al., 3D Bioprinting of Vascularized, Heterogeneous Cell-laden Tissue Constructs, (2014), pp. 3124–3130, <https://doi.org/10.1002/adma.201305506>.
- [81] R.R. Jose, M.J. Rodriguez, T.A. Dixon, F. Omenetto, D.L. Kaplan, Evolution of bioinks and additive manufacturing technologies for 3D bioprinting, *ACS Biomater. Sci. Eng.* 2 (10) (2016) 1662–1678.
- [82] W.C. Wilson, T. Boland, Cell and organ printing 1: protein and cell printers, *Anat. Rec.* 272 (2) (2003) 491–496.
- [83] I.D. Ursan, L. Chiu, A. Pierce, Three-dimensional drug printing: a structured review, *J. Am. Pharm. Assoc.* 53 (2) (2013) 136–144.
- [84] A. Butscher, M. Bohner, S. Hofmann, L. Gauckler, R. Müller, Structural and material approaches to bone tissue engineering in powder-based three-dimensional printing, *Acta Biomater.* 7 (3) (2011) 907–920.
- [85] S.F.S. Shirazi, S. Gharehkhani, M. Mehrali, H. Yarmand, H.S.C. Metselaar, N.A. Kadri, N.A.A. Osman, A review on powder-based additive manufacturing for tissue engineering: selective laser sintering and inkjet 3D printing, *Sci. Technol.*

- Adv. Mater. 16 (3) (2015) 033502.
- [86] P.Y.V. Leung, Sugar 3D printing: additive manufacturing with molten sugar for investigating molten material fed printing, *3D Print. Addit. Manuf.* 4 (1) (2017) 13–18.
- [87] S.H. Jariwala, G.S. Lewis, Z.J. Bushman, J.H. Adair, H.J. Donahue, 3d printing of personalized artificial bone scaffolds, *3D Print. Addit. Manuf.* 2 (2) (2015) 56–64.
- [88] B. Nan, X. Yin, L. Zhang, L. Cheng, Three-dimensional printing of Ti<sub>3</sub>SiC<sub>2</sub>-based ceramics, *J. Am. Ceram. Soc.* 94 (4) (2011) 969–972.
- [89] J.A. Inzana, D. Olvera, S.M. Fuller, J.P. Kelly, O.A. Graeve, E.M. Schwarz, S.L. Kates, H.A. Awad, 3D printing of composite calcium phosphate and collagen scaffolds for bone regeneration, *Biomaterials* 35 (13) (2014) 4026–4034.
- [90] Z. Fu, L. Schlier, N. Travitzky, P. Greil, Three-dimensional printing of SiSiC lattice truss structures, *Mater. Sci. Eng. C* 560 (2013) 851–856.
- [91] S. Tasoglu, U. Demirci, Bioprinting for stem cell research, *Trends Biotechnol.* 31 (1) (2013) 10–19.
- [92] F. Obregon, C. Vaquette, S. Ivanovski, D.W. Huttmacher, L.E. Bertassoni, Three dimensional bioprinting for regenerative dentistry and craniofacial tissue engineering, *J. Dent. Res.* 94 (9,suppl) (2015) 143S–152S.
- [93] R. Suntornnond, J. An, C.K. Chua, Bioprinting of thermoresponsive hydrogels for next generation tissue engineering: a review, *Macromol. Mater. Eng.* 302 (1) (2017).
- [94] L. Meseguer-Olmo, V. Vicente-Ortega, M. Alcaraz-Baños, J.L. Calvo-Guirado, M. Vallet-Regí, D. Arcos, A. Baeza, In-vivo behavior of Si-hydroxyapatite/poly-caprolactone/DMB scaffolds fabricated by 3D printing, *J. Biomed. Mater. Res. A* 101 (7) (2013) 2038–2048.
- [95] U. Gbureck, T. Hölzel, U. Klammert, K. Würzler, F.A. Müller, J.E. Barralet, Resorbable dicalcium phosphate bone substitutes prepared by 3D powder printing, *Adv. Funct. Mater.* 17 (18) (2007) 3940–3945.
- [96] R. Trombetta, J.A. Inzana, E.M. Schwarz, S.L. Kates, H.A. Awad, 3D printing of calcium phosphate ceramics for bone tissue engineering and drug delivery, *Ann. Biomed. Eng.* 45 (1) (2017) 23–44.
- [97] A.V. Do, B. Khorsand, S.M. Geary, A.K. Salem, 3D printing of scaffolds for tissue regeneration applications, *Adv. Healthc. Mater.* 4 (12) (2015) 1742–1762.
- [98] A.L. Rutz, K.E. Hyland, A.E. Jakus, W.R. Burghardt, R.N. Shah, A multi material bioink method for 3D printing tunable, cell-compatible hydrogels, *Adv. Mater.* 27 (9) (2015) 1607–1614.
- [99] N. Raja, H.S. Yun, A simultaneous 3D printing process for the fabrication of bio-ceramic and cell-laden hydrogel core/shell scaffolds with potential application in bone tissue regeneration, *J. Mater. Chem. B* 4 (27) (2016) 4707–4716.
- [100] S. Ling, Q. Zhang, D.L. Kaplan, F. Omenetto, M.J. Buehler, Z. Qin, Printing of stretchable silk membranes for strain measurements, *Lab Chip* 16 (13) (2016) 2459–2466.
- [101] Y. Han, C. Wei, J. Dong, Droplet formation and settlement of phase-change ink in high resolution electrohydrodynamic (EHD) 3D printing, *J. Manuf. Process.* 20 (2015) 485–491.
- [102] J. Wang, M. Yang, Y. Zhu, L. Wang, A.P. Tomsia, C. Mao, Phage nanofibers induce vascularized osteogenesis in 3D printed bone scaffolds, *Adv. Mater.* 26 (29) (2014) 4961–4966 (2014).
- [103] J.P. Temple, D.L. Hutton, B.P. Hung, P.Y. Huri, C.A. Cook, R. Kondragunta, X. Jia, W.L. Grayson, Engineering anatomically shaped vascularized bone grafts with hASCs and 3D-printed PCL scaffolds, *J. Biomed. Mater. Res. A* 102 (12) (2014) 4317–4325.
- [104] N. Bizzotto, A. Sandri, D. Regis, D. Romani, I. Tami, B. Magnan, Three-dimensional printing of bone fractures: a new tangible realistic way for preoperative planning and education, *Surg. Innov.* 22 (5) (2015) 548–551.
- [105] C.L. Ventola, Medical applications for 3D printing: current and projected uses, *Pharm. Ther.* 39 (10) (2014) 704.
- [106] M.M. Barak, M.A. Black, A novel use of 3D-printing demonstrates structural effects of osteoporosis on cancellous bone stiffness and strength, *J. Mech. Behav. Biomed. Mater.* 78 (2018) 455–464.
- [107] J. Edwards, T. Rogers, The accuracy and applicability of 3D modeling and printing blunt force cranial injuries, *J. Forensic Sci.* 63 (3) (2018) 683–691.
- [108] T. Peng, Analysis of energy utilization in 3d printing processes, *Procedia CIRP* 40 (2016) 62–67.
- [109] M. Lee, H.Y. Kim, Toward nanoscale three-dimensional printing: nanowalls built of electrospun nanofibers, *Langmuir* 30 (5) (2014) 1210–1214.
- [110] L. Qin, D.C. Li, C. Cheng, W.J. Zhang, Y.X. Liu, Tissue-engineered soft tissue oriented manufacturing technologies and additive manufacturing, *Chin J Tissue Eng Res* 18 (8) (2014) 1263–1269.
- [111] V. Mironov, V. Kasyanov, R.R. Markwald, Organ printing: from bioprinter to organ biofabrication line, *Curr. Opin. Biotechnol.* 22 (5) (2011) 667–673.
- [112] D.B. Kolesky, R.L. Truby, A.S. Gladman, T.A. Busbee, K.A. Homan, J.A. Lewis, 3D bioprinting of vascularized, heterogeneous cell-laden tissue constructs, *Adv. Mater.* 26 (19) (2014) 3124–3130.
- [113] S. Michael, H. Sorg, C.T. Peck, L. Koch, A. Deiwick, B. Chichkov, et al., Tissue engineered skin substitutes created by laser-assisted bioprinting form skinlike structures in the dorsal skin fold chamber in mice, *PLoS One* 8 (3) (2013) e57741.
- [114] M.S. Mannoor, Z. Jiang, T. James, Y.L. Kong, K.A. Malatesta, W.O. Soboyejo, et al., 3D printed bionic ears, *Nano Lett.* 13 (6) (2013) 2634–2629.
- [115] N.E. Fedorovich, W. Schuurman, H.M. Wijnberg, et al., Biofabrication of osteochondral tissue equivalents by printing topologically defined, cell-laden hydrogel scaffolds, *Tissue Eng. Part C* 18 (1) (2012) 33–44.
- [116] K. Kim, C.H. Lee, B.K. Kim, et al., Anatomically shaped tooth and periodontal regeneration by cell homing, *J. Dent. Res.* 89 (8) (2010) 842–847.
- [117] J.Y. Kim, X. Xin, E.K. Moiola, et al., Regeneration of dental-pulp-like tissue by chemotaxis-induced cell homing, *Tissue Eng. Part A* 16 (10) (2010) 3023–3031.
- [118] C.H. Park, H.F. Rios, Q. Jin, et al., Biomimetic hybrid scaffolds for engineering human tooth-ligament interfaces, *Biomaterials* 31 (23) (2010) 5945–5952.
- [119] A.D. Metcalfe, M.W. Ferguson, Tissue engineering of replacement skin: the crossroads of biomaterials, wound healing, embryonic development, stem cells and regeneration, *J. R. Soc. Interface* 4 (14) (2007) 413–437.
- [120] Y. Kitagawa, Y. Naganuma, Y. Yajima, et al., Patterned hydrogel microfibers prepared using multilayered microfluidic devices for guiding network formation of neural cells, *Biofabrication* 6 (3) (2014) 035011, <https://doi.org/10.1088/1758-5082/6/3/035011>.
- [121] X. Li, J. He, W. Bian, et al., A novel silk-TCP-PEEK construct for anterior cruciate ligament reconstruction: an off-the shelf alternative to a bone-tendon-bone autograft, *Biofabrication* 6 (1) (2014) 015010, <https://doi.org/10.1088/1758-5082/6/1/015010>.
- [122] M. Vukicevic, B. Mosadegh, J.K. Min, et al., Cardiac 3D printing and its future directions, *JACC Cardiovasc. Imaging* 10 (2) (2017) 171–184, <https://doi.org/10.1016/j.jcmg.2016.12.001>.
- [123] W. Quan, 3D-printed Alginate/Hydroxyapatite Hydrogel in Combination of Atsstrin to Repair Bone Defects [Dissertation]. Hangzhou, Zhejiang University, Chinese, 2015.
- [124] Y. Yan, S. Li, Z. Xiong, X.H. Wang, T. Zhang, R.J. Zhang, Fabrication technology of tissue engineering scaffold based on rapid prototyping, *J Mech Eng* 46 (5) (2010) 93–98.
- [125] K. Tappa, U. Jammalamadaka, Novel biomaterials used in medical 3D printing techniques, *J. Funct. Biomater.* 9 (2018) E17. Link: <https://bit.ly/2LEsNtp>.
- [126] A.P. McGuigan, M.V. Sefton, Design criteria for a modular tissue-engineered construct, *Tissue Eng.* 13 (5) (2007) 1079–1089.
- [127] G. Chai, Y. Zhang, Q.H. Liu, S.X. Ma, Q.X. Hu, L. Cui, et al., A pilot study of three dimensional printing of human bone marrow stem cells (hBMSCs), *Shanghai J Stomatol* 19 (1) (2010) (77–80 Chinese).
- [128] V. Mironov, C. Drake, X. Wen, Research project: Charleston bioengineered kidney project, *Biotechnol. J.* 1 (9) (2006) 903–905.